



# LUND UNIVERSITY

## Development of an automated method for display of ischemic myocardium from simulated electrocardiograms.

Galeotti, Lorian; Strauss, David G; Ubachs, Joey; Pahlm, Olle; Heiberg, Einar

*Published in:*  
Journal of Electrocardiology

*DOI:*  
[10.1016/j.jelectrocard.2008.12.007](https://doi.org/10.1016/j.jelectrocard.2008.12.007)

2009

[Link to publication](#)

*Citation for published version (APA):*  
Galeotti, L., Strauss, D. G., Ubachs, J., Pahlm, O., & Heiberg, E. (2009). Development of an automated method for display of ischemic myocardium from simulated electrocardiograms. *Journal of Electrocardiology*, 42, 204-212. <https://doi.org/10.1016/j.jelectrocard.2008.12.007>

*Total number of authors:*  
5

### General rights

Unless other specific re-use rights are stated the following general rights apply:  
Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

Read more about Creative commons licenses: <https://creativecommons.org/licenses/>

### Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

LUND UNIVERSITY

PO Box 117  
221 00 Lund  
+46 46-222 00 00





LUND UNIVERSITY  
Faculty of Medicine

---

LUP

*Lund University Publications*

Institutional Repository of Lund University

---

This is an author produced version of a paper published in Journal of electrocardiology. This paper has been peer-reviewed but does not include the final publisher proof-corrections or journal pagination.

Citation for the published paper:

Loriano Galeotti, David G Strauss, Joey Ubachs, Olle Pahlm, Einar Heiberg

Development of an automated method for display of ischemic myocardium from simulated electrocardiograms.

Journal of electrocardiology,

2009 Jan 19. [Epub ahead of print]

<http://dx.doi.org/10.1016/j.jelectrocard.2008.12.007>

Access to the published version may  
require journal subscription.

Published with permission from:  
Elsevier Science B.V., Amsterdam

**Development of an Automated Method for Display of Ischemic Myocardium from  
Simulated Electrocardiograms (DIMS-ECG)**

Short title: Display of Ischemic Myocardium from Simulated ECGs

Loriano Galeotti<sup>1,2</sup> [PhD](#), David G. Strauss<sup>1,3,4</sup> [BA](#), Joey F.A. Ubachs<sup>1</sup> [MD](#),  
Olle Pahlm<sup>1</sup> [MD PhD](#), Einar Heiberg<sup>1</sup> [PhD](#)

<sup>1</sup>Department of Clinical Physiology, Lund University Hospital, Lund, Sweden

<sup>2</sup>BIM Lab, Department of Systems and Computer Science, University of Florence, Firenze, Italy

<sup>3</sup>Division of Cardiology, Johns Hopkins University, Baltimore, MD, USA

<sup>4</sup>School of Medicine, Duke University, Durham, NC, USA

**Address Reprint Requests and Correspondence:**

Einar Heiberg, PhD

Department of Clinical Physiology

Lund University Hospital, S-221 85

Lund, Sweden

Telephone: +46-46-173137, Fax: +46-46-151769

E-mail: [einar.heiberg@med.lu.se](mailto:einar.heiberg@med.lu.se)

Word count: 4,287

**Financial Support:** DGS is supported by the Sarnoff Cardiovascular Research Foundation, EH and JFAU are supported by Swedish Research Council, Swedish Heart and Lung Foundation, and Region of Scania.

## **Abstract**

Background: Knowledge of the size and location of ischemic myocardium during acute coronary occlusion could provide decision support prior to reperfusion therapy. ECG scores based on the number of leads and the sum of ST-segment elevation have been unreliable in quantifying ischemia. We aimed to develop a new method to graphically Display Ischemic Myocardium from Simulated Electrocardiograms (DIMS-ECG) associated with known ischemic regions.

Methods: Twenty-one patterns of ischemia based on normal coronary anatomy were programmed into the freely available program ECGSIM ([www.ecgsim.org](http://www.ecgsim.org)). Minor variations of these patterns and five levels of ischemia severity produced 45,455 ECGs; 1,000 normal ECGs were also added. Given a *de novo* ECG (an ECG from a patient), ST-segment and T-wave measurements are compared to ECG measurements in the database. The closest 200 matches are selected and the corresponding ischemic areas are “averaged” to create a graphical display of the ischemic myocardium.

Results: Three patients are presented who underwent elective coronary angioplasty with continuous ECG recording and scintigraphically defined ischemic myocardium. Based on ECG analysis, the program graphically displays the ischemic myocardium with close agreement to the scintigraphic images. The program’s source code and the ECG database will be made freely available.

Conclusions: The DIMS-ECG method graphically displays ischemic myocardium from information contained in the 12-lead ECG based on a novel approach to use a large simulated database instead of rule or score based method. Following further development and testing, the DIMS-ECG method could be used to risk-stratify patients with acute myocardial infarction.

**Key Words:** ischemia, ECG simulation, display, database

## **Introduction**

Following acute coronary artery occlusion, the final infarct size depends on the duration of occlusion, the size of ischemic myocardium at risk and collateral coronary flow to the ischemic region (1,2). Acute myocardial infarction can be treated by invasive primary percutaneous coronary intervention (PCI) or noninvasive thrombolytic agents, depending on the availability of PCI centers (*i.e.* prehospital or community hospital thrombolytics or transfer to a PCI center) (3,4). Knowing the size of myocardium at risk of infarction upon patient presentation could stimulate further research into which subsets of patients might benefit more from certain therapeutic strategies.

In humans, myocardium at risk can be measured with single photon emission computed tomography (SPECT) (5). A radioactive technetium-based tracer is injected before opening of the occluded vessel, and SPECT imaging is performed within 3 hours. However, this requires continuous availability of a radioactive tracer, injection of the tracer in the setting of acute coronary occlusion, and scanning with a gamma camera (usually after reperfusion), which could interfere with patient care. Although the tracer is injected before opening of the artery, the location and size of the myocardium at risk is often not determined until after reperfusion therapy has been administered. Therefore, new clinical methods that quantify myocardium at risk before treatment need to be developed.

The standard 12-lead electrocardiogram (ECG), which is inexpensive and widely available, is the most frequently used diagnostic tool for detecting both acute and healed myocardial infarction. Prior studies have used the presence or absence and the sum of ST-

segment deviation in the 12-lead ECG to quantify myocardium at risk (6), however, the results have been unreliable when compared with SPECT (7). These approaches do not take into account the complex interactions that affect the body-surface electrocardiogram, which include that certain ventricular walls have greater effects on the ECG than others, that individual leads are at different distances from the heart and that electrical cancellation can occur (8).

In order to make sense of these complex interactions to quantify chronic infarcts, Selvester and colleagues used computer simulation of the electrical activity of the heart to develop a 12-lead ECG QRS-scoring system to quantify different size infarcts throughout the left ventricle (9). [A new, freely-available simulation program, ECGSim \(www.ecgsim.org\) uses a heart and thorax model measured by magnetic resonance images and takes into account the complex geometry and differences in conductivity between the myocardium, blood pool and lungs \(10\). We hypothesized that simulations using ECGSim could be used to study acute ischemia and develop methods to quantify myocardium at risk of infarction.](http://www.ecgsim.org) The aim of the paper was to develop an automated method that Graphically Displays Ischemic Myocardium associated with a patient ECG, from here on denoted as *de novo* ECG by comparing the electrocardiogram to a database of Simulated Electrocardiograms (DIMS-ECG method).

## **Methods**

In this study, we generated a database of simulated 12-lead ECGs associated with known areas of ischemia. Then, given a *de novo* ECG, measurements of ST-segment elevation and T-wave amplitude from each lead are extracted and compared to the same measurements from all ECGs in the database. The closest matches are combined and presented graphically on a polar plot, which is a method of displaying the LV. Figure 1 shows the relationship between displaying

ischemic myocardium (shaded area) from a left anterior descending (LAD) artery occlusion on a “Mercator projection” (Figure 1A) and a polar plot (Figure 1B). Each image shows the typical distribution of the coronary arteries and the division of the left ventricle into four walls. The same region of ischemia is shown on a three-dimensional depiction of the left and right ventricles in Figure 2 (right).

### *Development of the DIMS-ECG database*

We used the freely available simulation program ECGSIM ([www.ecgsim.org](http://www.ecgsim.org)) (10) to simulate ischemia and produce a database of the corresponding ECGs. ECGSIM allows the user to alter the transmembrane (action) potentials on the endocardium and epicardium in 257 nodes on the left and right ventricles (Figure 2). ECGSIM does take into account the position of the heart in the chest and that electrical cancellation can occur. Parameters for each node can be set manually or can be retrieved from a file. The resulting electrical changes can be viewed on body surface maps and 12-lead ECGs that can be saved to files. Ischemia was simulated by changing the action potentials to yield a delayed initiation of action potential upstroke (delayed depolarization), a depolarized resting potential (resulting in reduced action potential amplitude) and earlier repolarization (reduced action potential duration). Of note, two additional changes do occur during acute ischemia. There is a decrease in the action potential upstroke velocity (which is separate from the delay in the initiation of the upstroke) and a decrease in the maximum potential to which the cell depolarizes (further reducing action potential amplitude in addition to the depolarized resting potential) (11-13). The process of creating the DIMS-ECG database is shown in Figure 3 and can be summarized as follows:



### 1. *Defining different levels of ischemia*

Five different levels of ischemia severity were simulated; the different levels included both delaying depolarization time by 15, 15, 10, 10 and 8 milliseconds, reducing action potential duration, and reducing action potential amplitude to 50%, 80%, 85%, 90% and 93% of normal.

### 2. *Establishing basic ischemic regions*

Simulating all possible ischemic patterns with 257 nodes would result in  $6^{257}$  potential combinations (one normal level and 5 different levels of ischemia). This amount of simulation is not possible to handle and therefore limitations were set. As a first step, we decided which physiologically ischemic regions should be included in the database. The location and size of the simulated ischemic regions were selected based on coronary artery distributions as previously defined by Selvester (Figure 1) (9). We divided the coronary artery distributions into 10 basic regions. These were combined to produce small, medium and large regions of ischemia to obtain a total of 23 regions (Table 1).

### 3. *Expanding ischemic regions*

Variations of the regions were developed by slightly expanding the size of the ischemic area outside of the basic regions. The region was allowed to include one of the neighbour nodes to the nodes within the basic region. This resulted in 9091 unique patterns and in each of these patterns five different levels of ischemia were simulated, resulting in a total of 45,455 ECGs. In addition, 1,000 “normal” ECGs were added to the database by introducing small random modifications of the normal action potentials. Given a normal *de novo* ECG, the program has to be able to find enough normal samples in the database to correctly classify the ECG.

### *Using the DIMS-ECG database*

The steps involved in using the DIMS-ECG database are shown in Figure 4 and can be summarized as follows:

1. Given a *de novo* ECG, maximum and minimum T-wave amplitude and ST-segment amplitude at the J-point, J + 40 ms and J + 80 ms were extracted for each lead, which resulted in a total of 60 measurements (5 parameters in 12 leads) for that particular ECG. In the current implementation, additional parameters can be chosen from a set of 27 possible parameters. The same measurements were extracted from each ECG in the database. The parameter-extraction routine was based on the SignalAnalysis software developed by the Signal Processing Group (Department of Applied Electronics, Lund University, Lund, Sweden) (14).
2. A simple approach would be to compare the 60 *de novo* ECG measurements with the corresponding measurements for each ECG in the database. However, many of these 60 measurements are highly correlated and, therefore, this approach would not result in an accurate method of matching two ECGs. Instead, the database was compressed by the use of Principal Component Analysis (PCA) (15). PCA finds orthogonal modes of variation in the database so that the 60 measurements from one ECG can accurately be described using only 3-5 parameters (principal components). In the current implementation of the algorithm the user can select the number of principal components to use.
3. The *de novo* ECG is compared to each ECG in the database by calculating the Euclidean distance between their principal coordinates. The closest 200 matches are selected and the regions of ischemia associated with the retrieved 200 matches are “averaged” to

obtain one image representing the myocardium at risk of infarction. This number of matches in the algorithm was selected to be approximately 5% of the number of ECGs in the database so that the matches would not exceed the number of combinations in one basic region. In addition, a percentage representing how many of the matched ECGs belonged to each basic region is calculated. This can be interpreted as the likelihood that the *de novo* ECG belongs to each basic region.

### ***Testing the simulated ECG database***

In order to test the applicability of the DIMS-ECG database, three patients were selected from the STAFF studies investigations (14, [16](#)). These individuals had stable coronary disease and were referred for prolonged percutaneous transluminal coronary angioplasty with nonperfusion balloons at the Charleston Area Medical Center (Charleston, West Virginia). The 3 patients were selected to have one example from each of the main coronary arteries that meets American College of Cardiology/American Heart Association ECG criteria for [acute](#) ST-elevation myocardial [ischemia](#). Patient #1 had a left circumflex (LCX) occlusion, patient #2 had a right coronary artery (RCA) occlusion and patient #3 had a left anterior descending (LAD) occlusion. They underwent two SPECT studies, one with sestamibi injection during prolonged balloon occlusion and one control study on the following day ([16](#)). The method for SPECT imaging acquisition and analysis was described previously ([16](#)). Twelve-lead ECGs were recorded continuously before, during and after angioplasty (14). For this study, we used ECGs recorded just before balloon deflation. The STAFF studies were approved by the investigational review board and informed consent was obtained from each subject.

## Results

Figure 5 shows the ECGs and Figure 6 shows the SPECT and DIMS-ECG polar plots for three patients who underwent prolonged coronary angioplasty. Patients #1 and #2 both have ECGs with ST-elevation in the inferior leads (II, III and aVF) and ST-depression in the anterior precordial leads (primarily V2 and V3). The DIMS-ECG algorithm correctly predicted that Patient #1 had an LCX occlusion and Patient #2 had an RCA occlusion. The DIMS-ECG polar plot output of Patient #1 predicted ischemia in the posterolateral and inferior walls, which is concordant with the SPECT ischemic region. The 200 ECGs in the DIMS-ECG database that were most similar to the ECG of Patient #1 consisted of 78% dominant LCX, 11% nondominant LCX and 11% RCA. The DIMS-ECG polar plot output of Patient #2 predicted ischemia limited to the inferior wall, which is in agreement with SPECT. The DIMS-ECG distribution of most-similar ECGs were 84% RCA and 16% dominant LCX. The LAD occlusion of Patient #3 produced ST-elevation in leads V2, V3, V4, I and aVL and ST-depression in leads III and aVF. The DIMS-ECG polar plot predicted ischemia in the anterosuperior and anteroseptal left ventricular wall, which is in agreement with SPECT. The 200 most similar ECGs (100%) were from LAD occlusion.

The entire algorithm is written in Matlab (<http://www.mathworks.com>) and will be made freely available in open source form upon the time of publication at <http://www.heiberg.se/dims-ecg>. This will also include the database with the 46,455 ECGs together with their classification and perfusion defect territories. The user can easily define a wide range of ECG parameters to include in the analysis and it is easy to recompute the PCA. The parameters can then be explored quantitatively. It is also possible to load ECGs and visualize their parametric time series.

## Discussion

We have developed an automated algorithm to quantify and graphically display ischemic myocardium at risk of infarction. The novel DIMS-ECG method uses the freely available ECG simulation program ECGSIM to create a database of approximately 45,000 ECGs paired with graphical displays of ischemia. Given a *de novo* ECG, ST-segment and T-wave amplitude measurements are compared with those of the ECGs in the database. Similar ECGs are identified and their graphical displays of ischemia are averaged to show the estimated ischemic area for the *de novo* ECG. Following further development and testing, this DIMS-ECG method could be implemented in commercial ECG machines and used to risk-stratify patients with acute myocardial infarction in the prehospital or emergency department setting.

Physicians and researchers have been using the ECG to diagnose myocardial ischemia and infarction for almost 100 years. However, it is difficult to unscramble the complex interactions that affect the body-surface ECG. In the 1950s-1960s there were conflicting studies in the literature regarding the ability of the ECG to diagnose chronic infarcts (17). However, computer simulation of electrical depolarization by Selvester and colleagues showed that infarcts in all parts of the heart produced quantifiable changes in the body-surface ECG (17,18). This led to the development of the 53-criteria, 32-point Selvester QRS-score to quantify and localize infarcts (9). While the ECG is routinely used to diagnose acute myocardial ischemia, there have been conflicting reports regarding its ability to quantify the size of ischemic myocardium (6,7). Prior approaches have not been based on systematic simulation of ischemia and have used simplistic approaches where ST-segment deviation in each lead is given equal weight. This does not take into account that individual ECG leads are at different distances from the heart and that

certain ventricular walls have greater effects on the ECG. Thus, we sought to develop a more sophisticated algorithm by simulating different sizes and severities of ischemia throughout the LV. However, unlike the rule-based approach developed by Selvester (18), we have created a database of approximately 45,000 simulated ECGs connected to maps of the associated ischemic region. The automated computer algorithm (DIMS-ECG) uses PCA to compare a *de novo* ECG to all ECGs in the database and identifies the 200 closest ECGs. DIMS-ECG then superimposes the 200 ischemia maps to display the predicted ischemia location and the predicted coronary artery that is occluded.

The freely available DIMS-ECG algorithm together with the ECG database may be useful for a large number of studies. The software will allow other researchers to continue the approach of simulating ECGs to test various analysis schemes and to explore different parameters for quantifying and graphically displaying ischemic myocardium. For example, as ischemia continues and necrosis develops, ST-segment and T-wave changes may decrease in magnitude, and QRS changes such as pathological Q waves will likely develop. This would result in underestimation of the ischemia region by the current DIMS-ECG algorithm. Future work should include simulation of electrically inactive cells and analysis of QRS complex measurements [to simulate effects of confounding prior infarcts](#). Such an approach may allow prediction and graphical display of myocardium that is already dead and myocardium that is ischemic, but potentially salvageable following reperfusion. Prior studies have indicated that information regarding the potential for myocardial salvage is contained in the 12-lead ECG (19).

Limitations of the current version of the DIMS-ECG database are that it was based on simulations from a single heart's and thorax's geometry. Simulating ECGs using different heart positions, angles and geometries may improve the ability of the DIMS-ECG algorithm to

quantify and localize ischemic myocardium. In addition, the normal values for 12-lead ECGs are known to differ by age, gender and race (20). Inputting normal ECGs into the database classified by these variables, and then adding these as input variables when analyzing a *de novo* ECG, may improve the algorithm's performance. Finally, further study is required to validate the DIMS-ECG method against other measures of ischemic myocardium (*e.g.* SPECT) in patients. Unfortunately, SPECT imaging has its own limitations and, thus, any method to quantify and display ischemic myocardium should be prospectively studied to determine if it provides additional value in risk-stratifying patients with acute myocardial infarction.

In conclusion, we have presented a method where an ECG from a patient with potential ischemia can be compared to a database of simulated ECGs associated with known areas of ischemia. This DIMS-ECG program identifies similar ECGs in the database and outputs a graphical display of the predicted ischemic myocardium for the *de novo* ECG. The program and associated database will be made freely available for further development and testing.

## **Acknowledgements**

The authors wish to acknowledge valuable help from Dr. Thom Oostendorp, University of Nijmegen, the Netherlands regarding ECGSSIM and from Professor Leif Sörmo, Lund University, for comments on the DIMS-ECG algorithm development.

## References

1. Reimer KA, Jennings RB, Cobb FR, Murdock RH, Greenfield JC, Jr., Becker LC, Bulkley BH, Hutchins GM, Schwartz RP, Jr., Bailey KR, et al. Animal models for protecting ischemic myocardium: results of the NHLBI Cooperative Study. Comparison of unconscious and conscious dog models. *Circ Res.* 1985; 56:651-665.
2. Christian TF, Schwartz RS, Gibbons RJ. Determinants of infarct size in reperfusion therapy for acute myocardial infarction. *Circulation.* 1992; 86:81-90.
3. Antman EM, Hand M, Armstrong PW, Bates ER, Green LA, Halasyamani LK, Hochman JS, Krumholz HM, Lamas GA, Mullany CJ, Pearle DL, Sloan MA, Smith SC, Jr., Anbe DT, Kushner FG, Ornato JP, Jacobs AK, Adams CD, Anderson JL, Buller CE, Creager MA, Ettinger SM, Halperin JL, Hunt SA, Lytle BW, Nishimura R, Page RL, Riegel B, Tarkington LG, Yancy CW. 2007 focused update of the ACC/AHA 2004 guidelines for the management of patients with ST-elevation myocardial infarction: a report of the American College of Cardiology/American Heart Association task force on practice guidelines: developed in collaboration with the Canadian Cardiovascular Society endorsed by the American Academy of Family Physicians: 2007 writing group to review new evidence and update the ACC/AHA 2004 guidelines for the management of patients with ST-elevation myocardial infarction, writing on behalf of the 2004 writing Committee. *Circulation.* 2008; 117:296-329.
4. Ting HH, Krumholz HM, Bradley EH, Cone DC, Curtis JP, Drew BJ, Field JM, French WJ, Gibler WB, Goff DC, Jacobs AK, Nallamothu BK, O'Connor RE, Schuur JD. Implementation and integration of prehospital ecgs into systems of care for acute



- coronary syndrome. A scientific statement from the American Heart Association interdisciplinary council on quality of care and outcomes research, emergency cardiovascular care committee, council on cardiovascular nursing, and council on clinical cardiology. *Circulation*. 2008; 118:1066-1079.
5. Sinusas AJ, Trautman KA, Bergin JD, Watson DD, Ruiz M, Smith WH, Beller GA. Quantification of area at risk during coronary occlusion and degree of myocardial salvage after reperfusion with technetium-99m methoxyisobutyl isonitrite. *Circulation*. 1990; 82:1424-1437.
  6. Aldrich HR, Wagner NB, Boswick J, Corsa AT, Jones MG, Grande P, Lee KL, Wagner GS. Use of initial ST-segment deviation for prediction of final electrocardiographic size of acute myocardial infarcts. *Am J Cardiol*. 1988; 61:749-753.
  7. Christian TF, Gibbons RJ, Clements IP, Berger PB, Selvester RH, Wagner GS. Estimates of myocardium at risk and collateral flow in acute myocardial infarction using electrocardiographic indexes with comparison to radionuclide and angiographic measures. *J Am Coll Cardiol*. 1995; 26:388-393.
  8. Holland RP, Brooks H, Lidl B. Spatial and nonspatial influences on the TG-ST segment deflection of ischemia. Theoretical and experimental analysis in the pig. *J Clin Invest*. 1977; 60:197-214.
  9. Selvester RH, Wagner GS, Ideker RE. Myocardial Infarction. In: Macfarlane PW, Lawrie TDV, eds. *Comprehensive electrocardiology: theory and practice in health and disease*. Vol 1. New York: Pergamon Press; 1989:565-629.

10. van Oosterom A, Oostendorp TF. ECGSIM: an interactive tool for studying the genesis of QRST waveforms. *Heart*. 2004; 90:165-168.
11. Kleber AG, Janse MJ, van Capelle FJ, Durrer D. Mechanism and time course of S-T and T-Q segment changes during acute regional myocardial ischemia in the pig heart determined by extracellular and intracellular recordings. *Circ Res*. 1978; 42:603-613.
12. Shaw RM, Rudy Y. Electrophysiologic effects of acute myocardial ischemia: a theoretical study of altered cell excitability and action potential duration. *Cardiovasc Res*. 1997; 35:256-272.
13. Miller WT, 3rd, Geselowitz DB. Simulation studies of the electrocardiogram. II. Ischemia and infarction. *Circ Res*. 1978; 43:315-323.
14. Persson E, Pettersson J, Ringborn M, Sornmo L, Warren SG, Wagner GS, Maynard C, Pahlm O. Comparison of ST-segment deviation to scintigraphically quantified myocardial ischemia during acute coronary occlusion induced by percutaneous transluminal coronary angioplasty. *Am J Cardiol*. 2006; 97:295-300.
15. [Jolliffe I.T. Principal Component Analysis, Series: Springer Series in Statistics, 2nd ed., Springer, NY, ISBN 978-0-387-95442-4, 2002.](#)
16. Persson E, Palmer J, Pettersson J, Warren SG, Borges-Neto S, Wagner GS, Pahlm O. Quantification of myocardial hypoperfusion with <sup>99m</sup>Tc-sestamibi in patients undergoing prolonged coronary artery balloon occlusion. *Nucl Med Commun*. 2002; 23:219-228.
17. Strauss DG, Selvester RH. The QRS complex -- a biomarker that "images" the heart: QRS scores to quantify myocardial scar in the presence of normal and abnormal ventricular conduction. *J Electrocardiol*. 2009; 42:(in press).

18. Selvester RH, Kalaba R, Collier CR, Bellman R, Kagiwada H. A digital computer model of the vectorcardiogram with distance and boundary effects: simulated myocardial infarction. *Am Heart J.* 1967; 74:792-808.
19. Sejersten M, Ripa RS, Maynard C, Grande P, Andersen HR, Wagner GS, Clemmensen P. Timing of ischemic onset estimated from the electrocardiogram is better than historical timing for predicting outcome after reperfusion therapy for acute anterior myocardial infarction: a DANish trial in Acute Myocardial Infarction 2 (DANAMI-2) substudy. *Am Heart J.* 2007; 154:61 e61-68.
20. Engblom H, Hedstrom E, Palmer J, Wagner GS, Arheden H. Determination of the left ventricular long-axis orientation from a single short-axis MR image: relation to BMI and age. *Clin Physiol Funct Imaging.* 2004; 24:310-315.

## Figure Legends

**Figure 1.** (A) Mercator projection of the LV. The LV has been divided into 10 basic regions that can potentially be infarcted based on regional coronary anatomy. The highlighted region shows the ischemic area (sections 1, 2 and 10) from an LAD occlusion that is distal to the first diagonal artery but proximal to the first septal perforator artery. (B) A polar plot of the LV. The same ischemic area from (A) is highlighted. LAD=left anterior descending, LCX=left circumflex, RCA=right coronary artery, PDA=posterior descending artery.



**Figure 2.** (A) Representation of the thorax, ventricles and action potentials from an epicardial node from ECGSIM ([www.ecgsim.org](http://www.ecgsim.org)). The left side shows a normal heart and action potential. The right side shows an ischemic area highlighted in green that is equivalent to the ischemic area from Figure 1. The ischemic action potential has delayed depolarization, early repolarization and decreased amplitude. (B) 12-lead ECGs resulting from the normal simulation (blue) and the ischemic simulation from the LAD occlusion depicted in (A). LV=left ventricle; RV=right ventricle; LAD=left anterior descending.

**Figure 3.** Development of the DIMS-ECG database. The 10 ischemic regions were combined to create 21 basic ischemic regions (see Table 1). Minor alterations were made to the basic ischemic regions to create 8819 ischemic patterns. Five different ischemia severity levels were simulated in each unique pattern to create 44,095 ECGs paired with known ischemia regions. LAD=left anterior descending; RCA=right coronary artery.

**Figure 4.** Using the DIMS-ECG database. ST-segment and T-wave amplitude measurements are extracted from the *de novo* ECG and compared to the same measurements from each ECG in the database using principal component analysis (PCA). The 200 closest ECG matches are identified and the corresponding ischemia maps are superimposed to create a map showing the predicted ischemia location. The percentage of the 200 matches from each coronary artery territory is also presented that can be used to predict the location of the occlusion.

**Figure 5.** 12 lead ECGs for 3 patients who underwent prolonged coronary angioplasty. ECGs were recorded prior to balloon deflation. Patient #1 had an left circumflex occlusion, Patient #2 had an right coronary artery occlusion and Patient #3 had an left anterior descending occlusion.

**Figure 6.** SPECT (left column) and DIMS-ECG (right column) polar plots for the same 3 patients as in Figure 5. Color scales show the distribution of ischemic to nonischemic myocardium for SPECT and the predicted ischemic to nonischemic scale for DIMS-ECG.

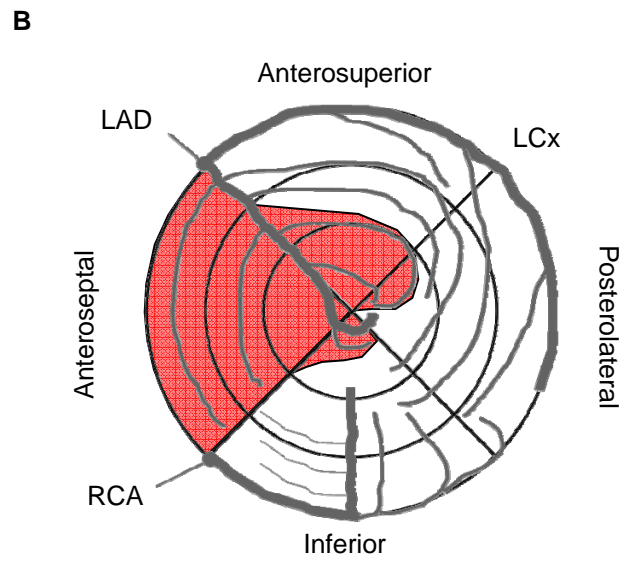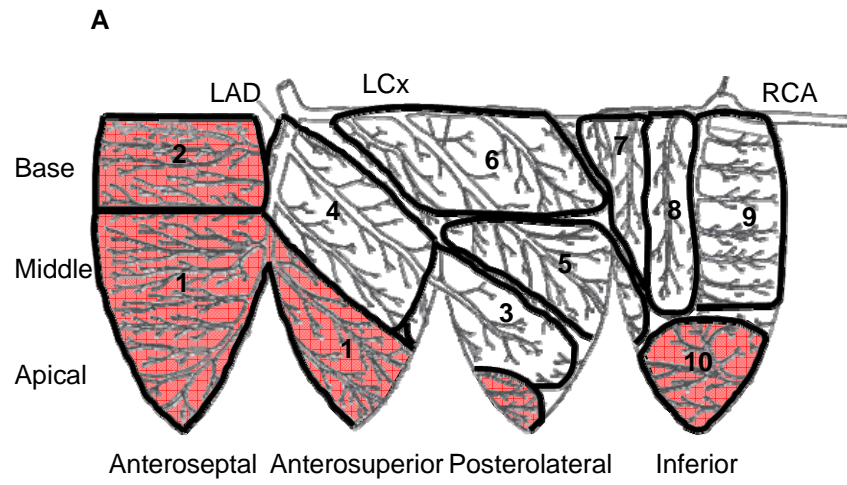

**Figure 1.**

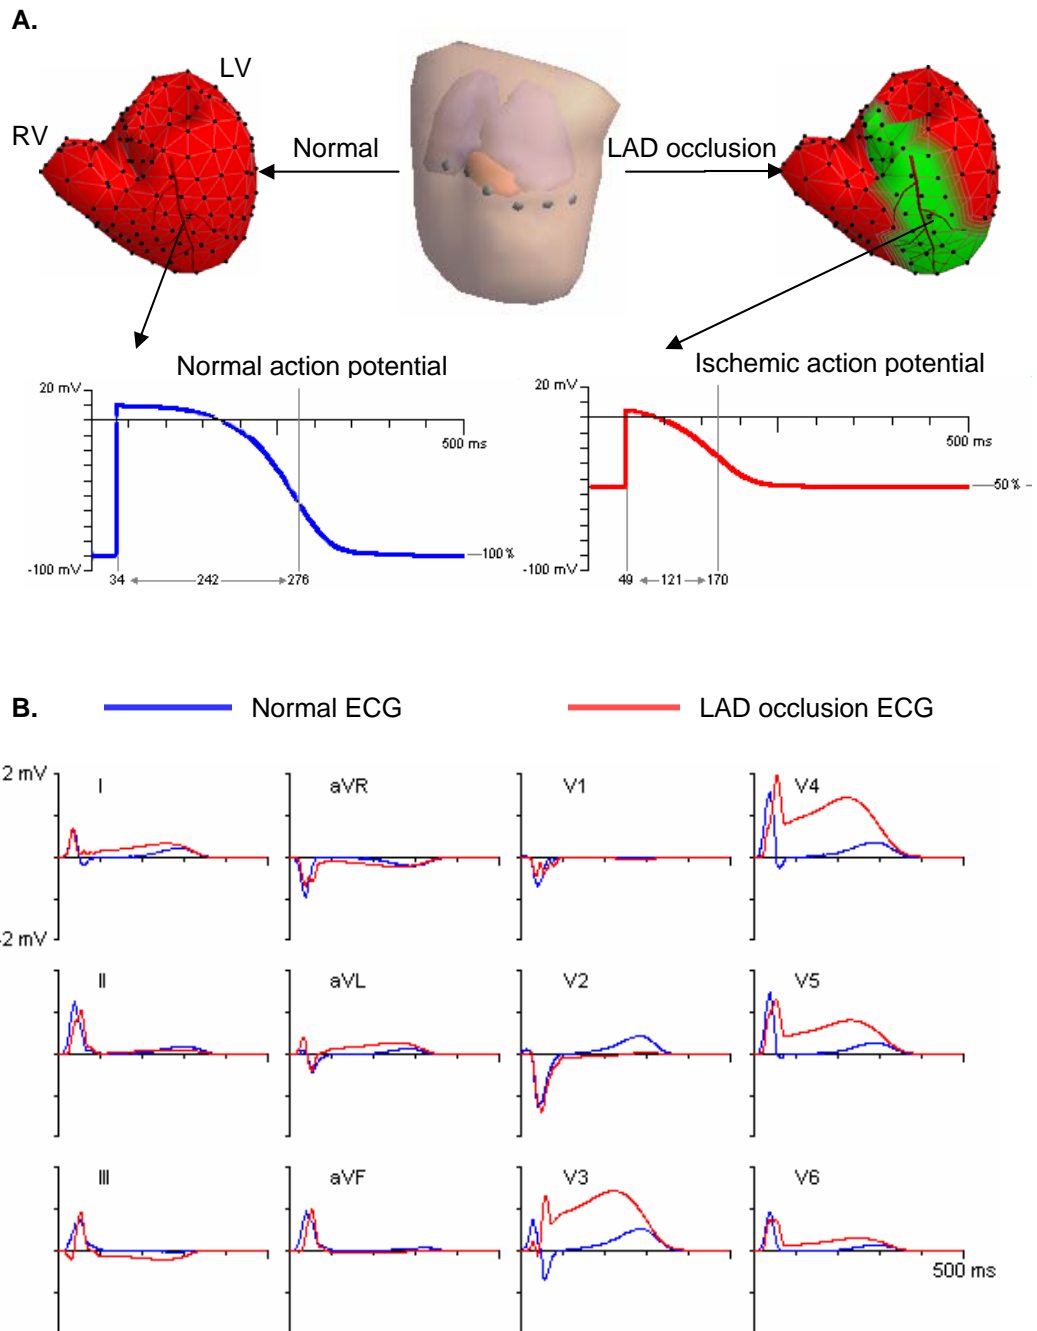


Figure 2.

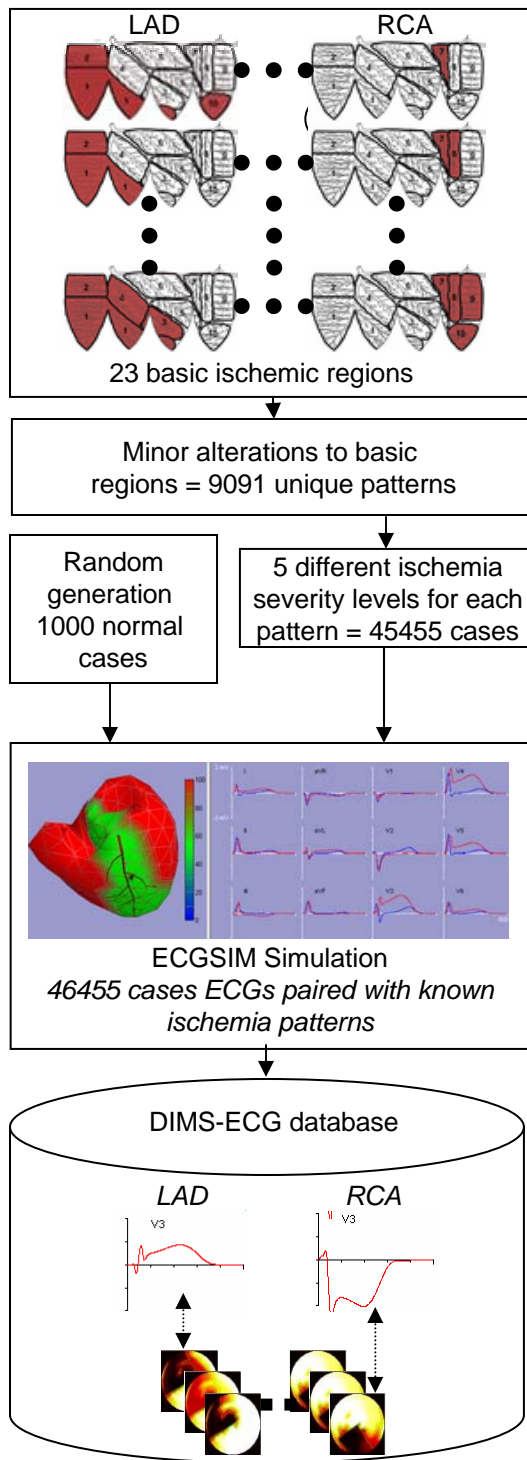


Figure 3.



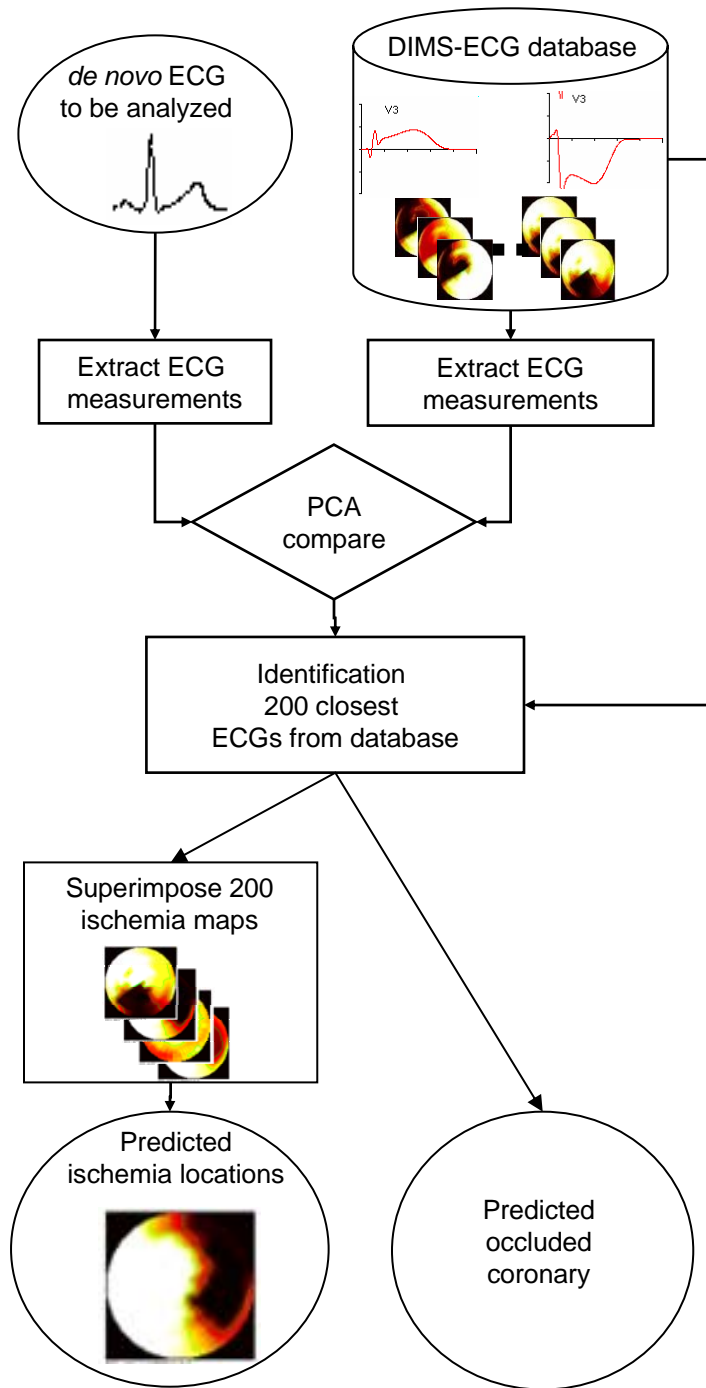


Figure 4.

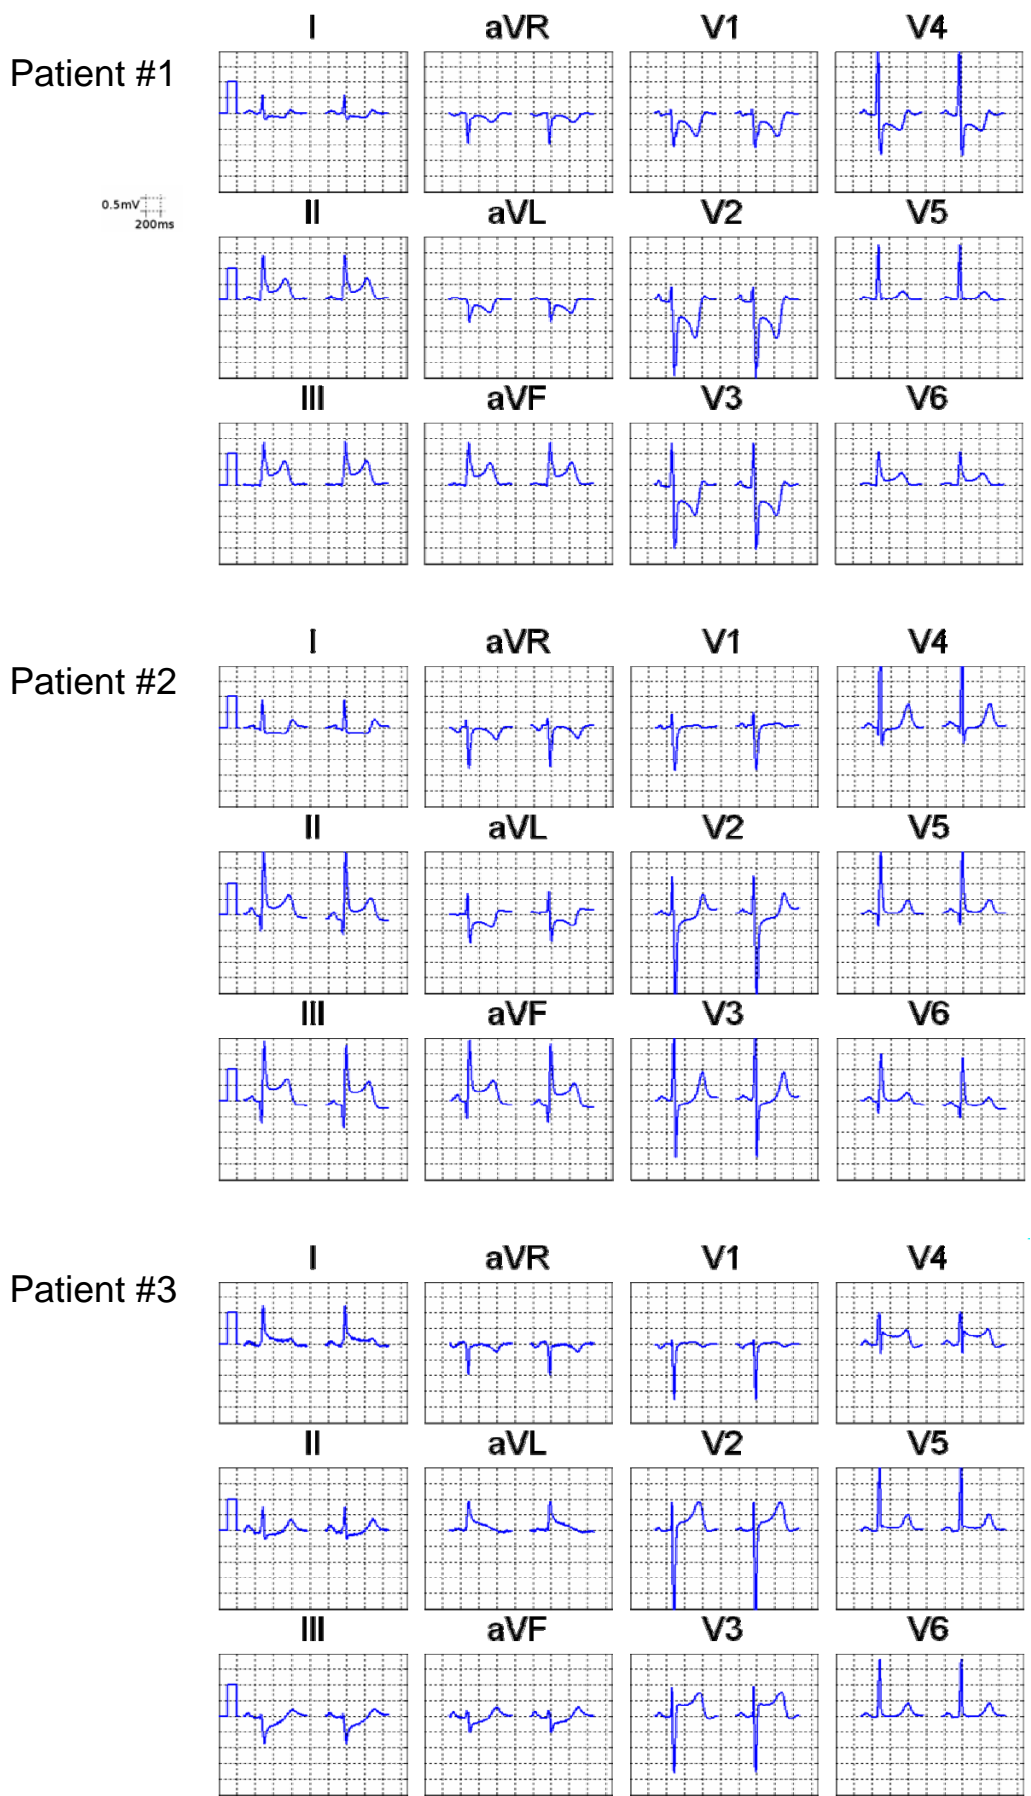


Figure 5.

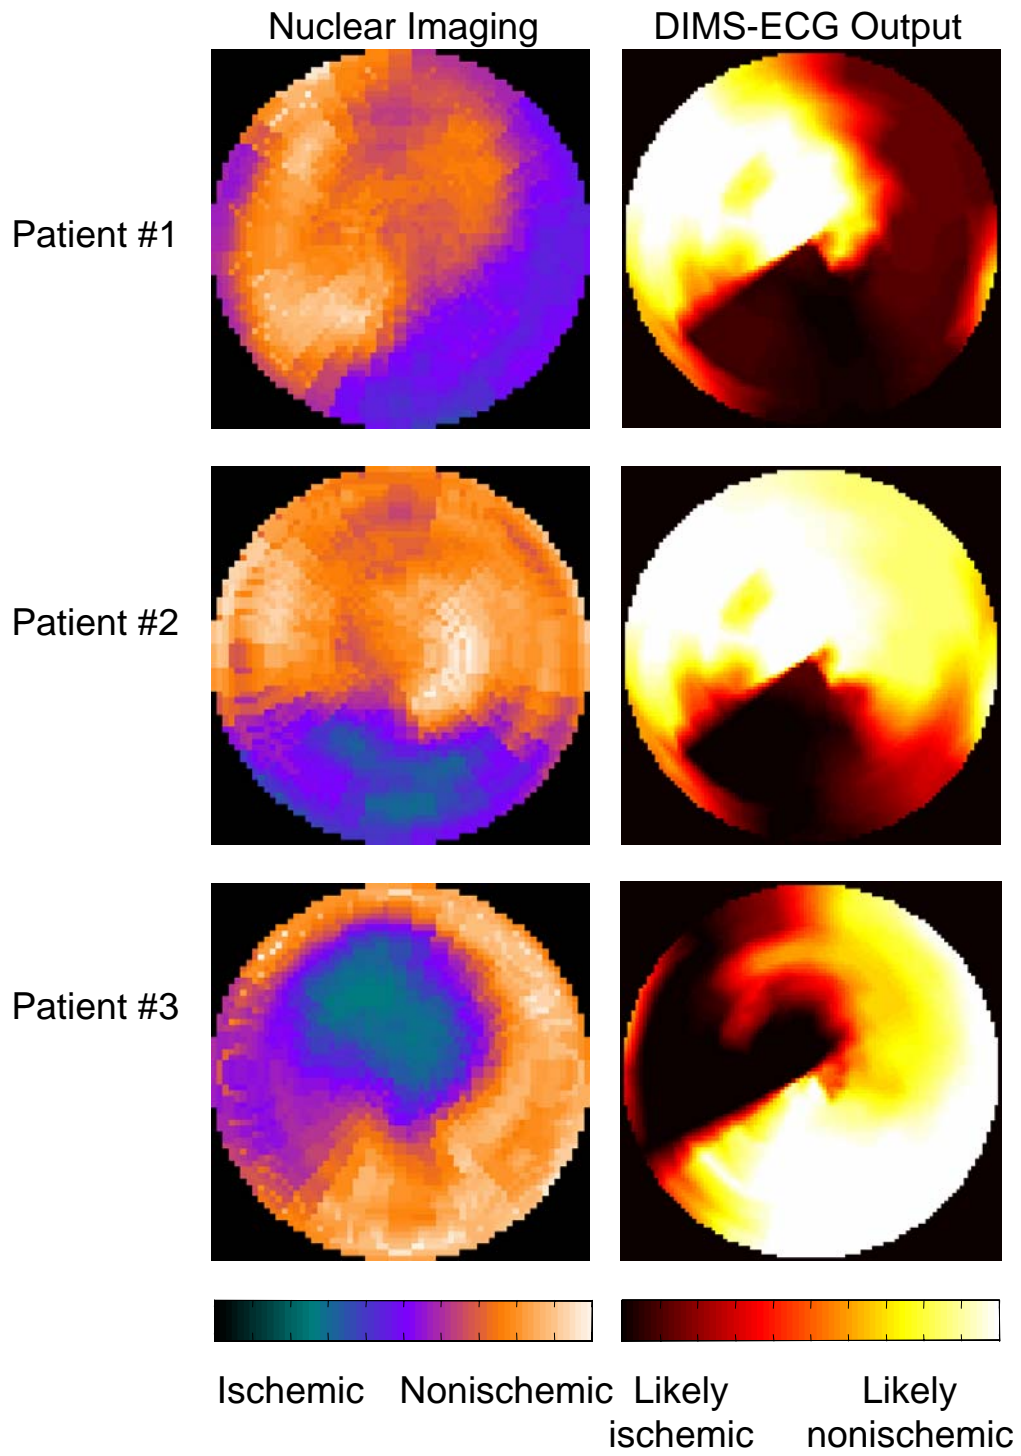


Figure 6.