



LUND UNIVERSITY

Simultaneous Spatially Resolved No and No₂ Measurements Using One-photon and 2-photon Laser-induced Fluorescence

Aldén, Marcus; Edner, H; Wallin, S

Published in:
Optics Letters

DOI:
[10.1364/OL.10.000529](https://doi.org/10.1364/OL.10.000529)

1985

[Link to publication](#)

Citation for published version (APA):

Aldén, M., Edner, H., & Wallin, S. (1985). Simultaneous Spatially Resolved No and No₂ Measurements Using One-photon and 2-photon Laser-induced Fluorescence. *Optics Letters*, 10(11), 529-531.
<https://doi.org/10.1364/OL.10.000529>

Total number of authors:
3

General rights

Unless other specific re-use rights are stated the following general rights apply:
Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

Read more about Creative commons licenses: <https://creativecommons.org/licenses/>

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

LUND UNIVERSITY

PO Box 117
221 00 Lund
+46 46-222 00 00

Simultaneous spatially resolved NO and NO₂ measurements using one- and two-photon laser-induced fluorescence

Marcus Aldén, Hans Edner, and Svante Wallin

Lund Institute of Technology, Department of Physics, P.O. Box 118, S-221 00 Lund, Sweden

Received March 14, 1985; accepted August 28, 1985

We demonstrate how spatially resolved distributions of NO and NO₂ can be simultaneously detected by using a single laser pulse at 452 nm. The laser-induced fluorescence from NO was achieved by a two-photon transition in the γ band at 226 nm followed by UV detection, whereas NO₂ was detected by a one-photon transition followed by Stokes fluorescence.

Laser-induced fluorescence, LIF, is one of the most promising techniques for diagnostics of combustion processes, as described, e.g., in Ref. 1. By tuning a laser wavelength to an absorption line of a molecule or an atom, followed by detection of subsequent fluorescence radiation, it is possible to measure temperatures as well as low number densities for flame radicals, e.g., OH, CH, C₂, and CN.

During the past few years two major achievements have been made in the application of LIF to combustion studies. The first of these achievements was a technique yielding spatially resolved measurements, first in one dimension² by using a linear diode array, shortly followed by two-dimensional measurements utilizing a vidicon³ and a diode matrix.⁴ The imaging technique was also extended to two-species (C₂, OH) detection by using two separate laser systems.⁵ The second achievement was the introduction of multiphoton absorption processes, which made it possible to detect atoms and molecules, e.g., O, H, C, and CO, that absorb in the VUV spectral region and therefore are impossible to detect by a one-photon transition because of large molecular absorption at these wavelengths.

Much of the groundwork concerned with the detection of light atoms (O, N) was carried out by Bischel *et al.*⁶ under well-controlled conditions. This work was followed shortly by flame detection of O (Ref. 7) and H.^{8,9} The combination of imaging and multiphoton absorption LIF experiments was also recently reported for CO,¹⁰ O,¹¹ and H (Ref. 12) in a flame environment.

In this Letter we describe the simultaneous detection of NO and NO₂ by using one laser pulse at 452 nm. This wavelength induces a two-photon transition in the γ band at 226 nm of NO with subsequent fluorescence in the UV spectral region. NO was previously studied by using either a one-photon transition,^{13,14} or a two-photon transition,^{15,16} and imaging experiments of NO have been described by Kychakoff *et al.*¹⁷ NO₂ has an absorption band in the blue spectral region, and the fluorescence occurs in the visible region. LIF from NO₂ is complicated by the fact that the lifetime is quite long, $\sim 50 \mu\text{sec}$, which makes the quenching phe-

nomenon severe. However, Barnes and Kircher¹⁸ have used a laser wavelength between 450 and 470 nm, where the lifetimes are less than $1 \mu\text{sec}$,¹⁹ and they were able to observe fluorescence from NO₂ in a flame at atmospheric pressure.

With the global interest in NO_x as a major pollutant, we believe that the technique proposed in this Letter is of great value. It would be possible, e.g., to study the spatial conversion of NO into NO₂ in flames and turbulent flows. Here the technique is demonstrated in a cell. For a more realistic situation preliminary experiments were performed with a jet of NO in air, where the conversion of NO to NO₂ could be seen as a brownish discoloration. However, since we lacked proper ventilation conditions, these experiments were abandoned for reasons of health.

A diagram of the setup used in the measurements is shown in Fig. 1. A Quanta-Ray DCR-1A Nd:YAG laser together with a Quanta-Ray PDL-1 tunable dye laser was used. The dye laser was operated with Coumarin 2 dye (Lambda Physik), yielding an output energy level of about 5 mJ at 452 nm, the wavelength used for the one-photon transition in NO₂ and the two-photon transition in NO. Approximately 30% of

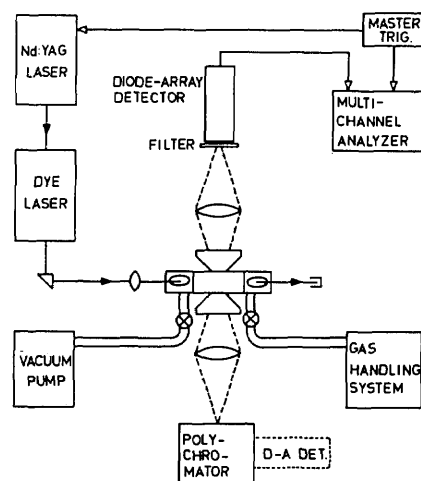


Fig. 1. Experimental setup. D-A DET., diode-array detector.

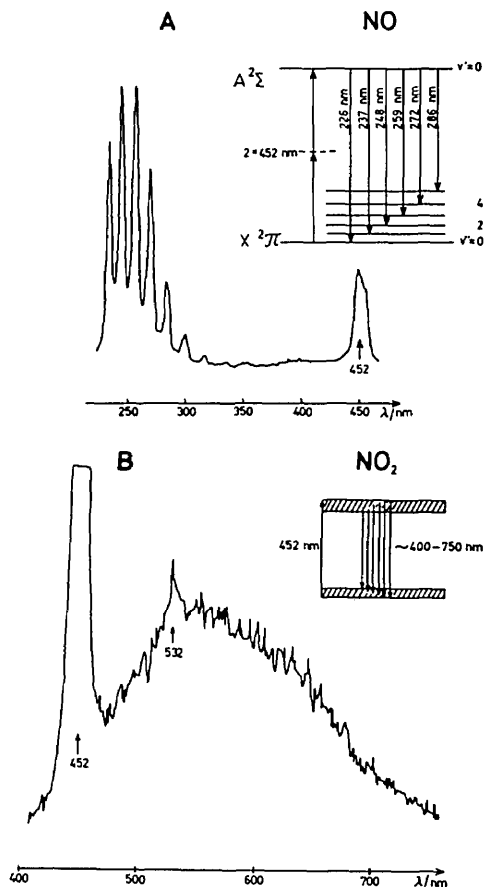


Fig. 2. LIF spectra of A, NO molecules and B, NO₂ molecules, with an excitation wavelength of about 452 nm. The relevant energy-level diagrams are inserted.

the output power was broadbanded because of amplified spontaneous emission. The dye-laser beam was focused into a cell with a lens ($f = 75 \text{ mm}$). The cell, with a volume of 24 cm^3 , was made of stainless steel and equipped with windows made of fused silica in order to minimize laser-induced fluorescence. A gas-handling system and a vacuum pump were connected to the cell so that various amounts of pure NO or NO-air/N₂ mixtures could be introduced.

The fluorescence radiation from the NO/NO₂ molecules was collected by a 50-mm-diameter $f/1$ quartz lens perpendicular to the laser beam. In the spectral measurements the light was focused onto the entrance slit of a Jarrell-Ash MonoSpec 18 that was used as a polychromator with a dispersion of 18 nm/mm (300 grooves/mm , blaze 300 nm). In the focal plane of the polychromator the light was detected by an EG&G PARC Model 1420 intensified diode-array detector.

In the imaging experiments the diode-array detector was placed directly in the image plane, after isolation of the interesting spectral region with optical filters. The diode-array detector was connected to the EG&G PARC Model 1218/1215 detector controller and multichannel analyzer, where the data were finally stored on diskettes. The detector was gated through a PARC Model 1211 high-voltage-pulse generator with a gate width of $1 \mu\text{sec}$.

In order for the appropriate filters for the imaging

experiments to be chosen, the spectral emission from NO and NO₂ was identified with the polychromator setup. Figure 2A shows the fluorescence spectrum of NO with an excitation wavelength of 452.16 nm . The fluorescence forms a progression from $v' = 0$ to $v'' = 0-7$ in the spectral region between 230 and 320 nm . The peak at 452 nm is due to scattered laser light in optical components. The fluorescence spectrum of NO₂, which is shown in Fig. 2B, lies on the low-energy side of the laser wavelength. The spectrum is broad and extends over the whole visible spectral region. Thus the light can easily be separated from the NO radiation, which is in the UV, with a cutoff filter. We used a Schott OG 590 filter, which also sufficiently suppressed the scattered laser light at 355 , 452 , and 532 nm . The NO fluorescence could be isolated with a solar-blind interference filter (Corion), which is transparent between 280 and 320 nm . We also used a Schott UG 11 filter, which is transparent for both NO and NO₂ fluorescence but suppresses scattered laser light.

A one-dimensional concentration distribution can be recorded if the laser beam, which gives rise to the fluorescence, is imaged directly onto a diode-array detector. Figure 3A shows a recording from a single pulse in $1000\text{-parts-in-}10^6$ (ppm) NO in N₂ in the cell at atmospheric pressure. Because of the relatively fast conversion of NO to NO₂, a steady stream of the calibration gas was passed through the cell.

The concentration of NO in the cell is thus uniform. The recording shows the behavior of a two-photon excitation the efficiency being dependent on the intensity squared, which gives rise to a higher signal from the focus of the laser beam. However, a more detailed study of the NO signal strength as a function of laser intensity in the focal point revealed a departure from the squared dependency at high laser power.

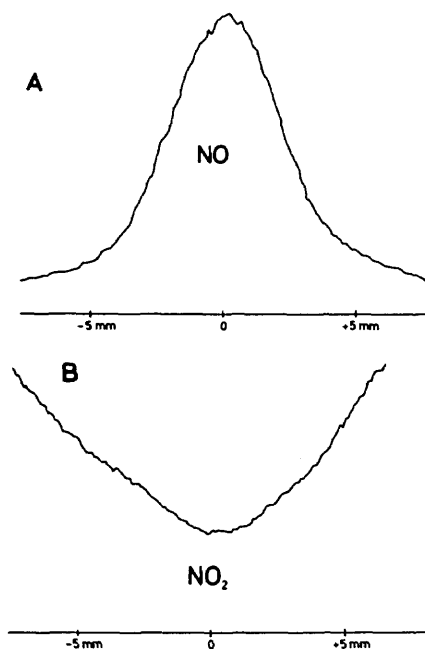


Fig. 3. One-dimensional single-shot image of the fluorescence distribution around the laser-beam focus for NO and NO₂, respectively.

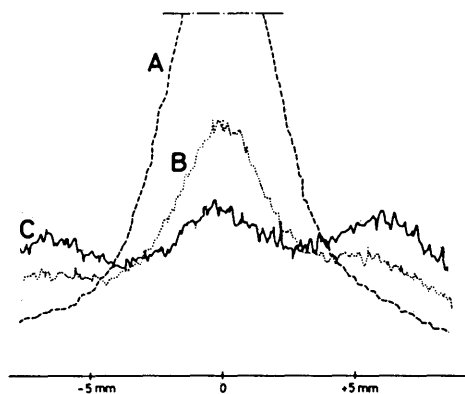


Fig. 4. Overlapping NO and NO₂ fluorescence distributions, captured in a single laser shot. A is a recording taken directly after filling the cell with a small amount of pure NO. B and C were taken with a time delay of 6 and 12 min, respectively.

At this point the signal dependence is closer to linear. According to Ref. 20, this phenomenon is more likely due to resonant Stark broadening than to a pure saturation effect.

In Fig. 3B the laser focus is imaged in the red spectral region with a small amount of NO₂ in the cell. Because of saturation effects the intensity decreases in the focus, although the NO₂ concentration is uniform in the cell. Thus, because of the one- and two-photon excitation, in the first case a greater signal is obtained outside the focus and in the second case most of the signal originates from the focus. These effects can be avoided by using a focusing lens with a longer focal length. In both Figs. 3A and 3B the peak signal intensity was ~1500 counts/pulse.

In order to examine the potential for practical measurements using this two-species approach, preliminary tests were performed yielding detectivity limits. Using the calibration gas with 1000 ppm of NO in N₂ followed by successive dilution, it was possible with the two-photon scheme to detect on the order of 1 ppm of NO at atmospheric pressure. By flowing 2000 ppm of NO₂ in air through the cell, we estimate a detection limit for NO₂ of the order of 100 ppm when using an excitation wavelength at 452 nm and a monochromator followed by a photomultiplier on the detection side. This number may seem surprisingly high since Ref. 18 gives the same detection limit with a laser power ~1000 times lower than ours. However, the use of a different and more favorable excitation wavelength, the saturation effect, and the detection by Barnes and Kircher of a very broadband wavelength distribution are probably the main reasons for the difference.

Figure 4 shows a recording from a single pulse of the somewhat overlapping fluorescence distributions from NO and NO₂ when a UG 11 filter was placed in front of the detector. The recordings were taken sequentially, every 6 min, after the cell was filled with a certain amount of pure NO at low pressure. The apparent transformation of NO to NO₂ is due to a small leakage of air into the cell and also to adsorption of NO on the cell walls followed by catalytic oxidation to NO₂.²¹

As has been demonstrated in this Letter, NO and NO₂ can be detected simultaneously by using only one laser pulse. This can be compared with our previous two-species LIF experiments,⁵ in which two completely different laser systems were used. In these experiments the two species (C₂ and OH) were detected separately by using a special mirror arrangement creating two images and different optical filters. This approach would also work in the present NO/NO₂ experiment, since the NO fluorescence occurs in the UV spectral region while the NO₂ fluorescence is found in the visible and toward the red spectral region.

The approach with linear array described here could of course easily be extended to two-dimensional images, as was recently shown by Cattolica.²²

The authors acknowledge the support of S. Svanberg and G. Holmstedt. This research was financially supported by The Swedish Institute of Gas Energy and by the Swedish Board for Technical Developments, STU.

References

1. See various papers in D. R. Crosley, ed., *Laser Probes for Combustion Chemistry* (American Chemical Society, Washington, D.C., 1980), pp. 61-207.
2. M. Aldén, H. Edner, G. Holmstedt, S. Svanberg, and T. Högberg, *Appl. Opt.* **21**, 1236 (1982).
3. M. J. Dyer and D. R. Crosley, *Opt. Lett.* **7**, 382 (1982).
4. G. Kychakoff, R. D. Howe, R. K. Hanson, and J. C. McDaniel, *Appl. Opt.* **21**, 3225 (1982).
5. M. Aldén, H. Edner, and S. Svanberg, *Appl. Phys.* **B29**, 93 (1982).
6. W. K. Bischel, B. E. Perry, and D. R. Crosley, *Appl. Opt.* **21**, 1419 (1982).
7. M. Aldén, H. Edner, P. Grafström, and S. Svanberg, *Opt. Commun.* **42**, 244 (1982).
8. R. P. Lucht, J. T. Salmon, G. B. King, D. W. Sweeney, and N. M. Laurendeau, *Opt. Lett.* **8**, 365 (1983).
9. M. Aldén, A. L. Schawlow, S. Svanberg, W. Wendt, and P.-L. Zhang, *Opt. Lett.* **9**, 211 (1984).
10. M. Aldén, S. Wallin, and W. Wendt, *Appl. Phys.* **B33**, 205 (1984).
11. M. Aldén, H. M. Hertz, S. Svanberg, and S. Wallin, *Appl. Opt.* **23**, 3255 (1984).
12. J. E. M. Goldsmith, *Opt. Lett.* **10**, 116 (1985); J. E. M. Goldsmith and R. J. M. Anderson, *Appl. Opt.* **24**, 607 (1985).
13. D. R. Grieser and R. H. Barnes, *Appl. Opt.* **19**, 741 (1980).
14. M. S. Chou, A. M. Dean, and D. Stern, *J. Chem. Phys.* **78**, 5962 (1983).
15. R. L. McKenzie and K. P. Gross, *Appl. Opt.* **20**, 2153 (1981).
16. T. Ozaki, Y. Matsui, and T. Ohsawa, *J. Appl. Phys.* **52**, 2593 (1981).
17. G. Kychakoff, K. Knapp, R. D. Howe, and R. K. Hanson, *AIAA J.* **22**, 153 (1984).
18. R. H. Barnes and J. F. Kircher, *Appl. Opt.* **17**, 1099 (1978).
19. P. B. Sacket and J. T. Yardley, *Chem. Phys. Lett.* **9**, 612 (1971).
20. K. P. Gross and R. L. McKenzie, *Opt. Lett.* **8**, 368 (1983).
21. B. Kasemo, Chalmers University of Technology, Göteborg, Sweden (personal communication).
22. R. J. Cattolica, Sandia National Laboratories, Albuquerque, N.M. 87185 (personal communication).