



LUND UNIVERSITY

Experimental Determination of Particle Deposition onto the Human Eye

Gudmundsson, Anders; Schneider, Thomas; Petersen, OH; Vinzents, PS; Bohgard, Mats; Akselsson, Roland

Published in:

Proceedings of NOSA and IV Finnish Aerosol Symposium, Finnish Meteorological Institute 1991

1991

[Link to publication](#)

Citation for published version (APA):

Gudmundsson, A., Schneider, T., Petersen, OH., Vinzents, PS., Bohgard, M., & Akselsson, R. (1991). Experimental Determination of Particle Deposition onto the Human Eye. *Proceedings of NOSA and IV Finnish Aerosol Symposium, Finnish Meteorological Institute 1991.*

Total number of authors:

6

General rights

Unless other specific re-use rights are stated the following general rights apply:

Copyright and moral rights for the publications made accessible in the public portal are retained by the authors and/or other copyright owners and it is a condition of accessing publications that users recognise and abide by the legal requirements associated with these rights.

- Users may download and print one copy of any publication from the public portal for the purpose of private study or research.
- You may not further distribute the material or use it for any profit-making activity or commercial gain
- You may freely distribute the URL identifying the publication in the public portal

Read more about Creative commons licenses: <https://creativecommons.org/licenses/>

Take down policy

If you believe that this document breaches copyright please contact us providing details, and we will remove access to the work immediately and investigate your claim.

LUND UNIVERSITY

PO Box 117
221 00 Lund
+46 46-222 00 00

**EXPERIMENTAL DETERMINATION OF PARTICLE DEPOSITION
ONTO THE HUMAN EYE.**

**A. GUDMUNDSSON,¹ T. SCHNEIDER,² O.H. PETERSEN,²
P.S. VINZENTS,² M. BOHGARD¹ AND K.R. AKSELSSON¹**

¹ Department of Working Environment, Lund Institute of Technology,
P.O. BOX 118, S-221 00 Lund, Sweden

² National Institute of Occupational Health, Lersø Parkallé 105,
D-2100 Copenhagen, Denmark

ABSTRACT

We perform studies of deposition of airborne particles onto the human eye. A mannequin with transparent and sticky foils covering its eyes is exposed to particles of fused alumina in a windtunnel. The airborne particle size distribution is simultaneously measured with an Aerodynamic Particle Sizer, APS. The particles on the foils are counted and measured with an optical microscope connected to an image analyzer.

Calibration between the APS determinations of particle size and number and the optical microscope determinations has been performed for particles of fused alumina.

KEYWORDS

deposition, human eye, windtunnel, aerodynamic particle sizer, optical microscope, particles of fused alumina,

INTRODUCTION

Deposition of particles onto human eyes is a problem in many areas for instance in connection with allergies and exposure to airborne man-made mineral fibers. The importance of deposition of particles onto the eyes is also discussed in connection with eye trouble when working in front of cathode ray tube displays.

The objective of the study is to investigate the mechanism of deposition of airborne particles onto the eyes. The experiments are done with a mannequin in a wind tunnel. The deposition rate dependence on parameters as air velocity, degree of turbulence, orientation to the air flow is determined.

The work is a cooperative project between the National Institute of Occupational Health, Denmark and the Lund Institute of Technology, Sweden.

METHODS

The deposition of airborne particles onto human eyes is studied in a wind tunnel. The cross sectional area of the wind tunnel is 1.1 m^2 . A mannequin with transparent and sticky foils covering its eyes is exposed to an aerosol. The powder used is fused alumina (grade designation F500, Washington Mills Electro Minerals Limited, Manchester, UK), and it is generated by a dispersion generator (RBG 1000, Palas GmbH, Karlsruhe, Germany). The airborne particle size distribution is simultaneously measured with an Aerodynamic Particle Sizer (APS model 3310, TSI, Inc., St. Paul, MN, USA), (Remiarz et al., 1983). The APS determine the aerodynamic particle diameter of the particles over the range $0.5 - 30 \text{ }\mu\text{m}$. The particles on the foils are counted and measured with an optical microscope (model Vanox-T, Olympus) connected to an image analyzer (model VIDAS, Kontron). The smallest particles are brought into focus and the projected area of each particle is determined with the optical microscope and the projected area diameter is calculated. Parameters that influence the deposition rate are studied. The air flow in the wind tunnel is operated at three air velocities $0.5, 1$ and 3 m/s . The mannequin is orientated at $0, 90$ and 180 degrees with respect to the forward-facing direction. At a air velocity of 1 m/s and the mannequin facing the wind, the influence of the degree of turbulence is investigated. The air velocity and degree of turbulence is measured with an anemometer system (IFA 100, TSI Inc). The results from the experiments are presented as deposition velocity as a function of the aerodynamic particle diameter and with the orientation of the mannequin, the air velocity and degree of turbulence as parameters.

To facilitate the use of optical microscopy measurements of the deposited particles and simultaneous measurements of the airborne particles with the APS, number and size calibration have to be performed. The calibration between the size determinations of the particles of fused alumina measured by the APS and the optical microscope is performed by determining the cutoff diameters for four impactors with both the instruments (Gudmundsson et al., 1991). The number calibration procedure is performed by sampling simultaneously with a membrane filter (filter type HAWP 02500, Millipore Corp., Massachusetts, USA) and with the APS. The particles are collected isokinetically and with thin-walled probes.

In the APS the particles accelerate through an orifice and pass two laser beams. The light scattered is detected and amplified with a single photomultiplier. Each particle creates a pair of pulses. Two signal processors working independently of each other, the small-particle processor (SPP) and the large-particle processor (LPP), measure the time difference between the pulses. The transit time is related to aerodynamic particle diameter through calibration with spheres of known geometric diameter and particle density. The SPP detect particles between $0.5 \text{ }\mu\text{m}$ and $15 \text{ }\mu\text{m}$ and the LPP between $5 \text{ }\mu\text{m}$ and $30 \text{ }\mu\text{m}$. There are a lot of counting rules for the SPP and the LPP, for instance the LPP and the SPP counts only particles if each pulse in the pulse pair have an amplitude greater than 3 V and 20 mV , respectively. In the APS several different case of coincidence effects occurs (Heitbrink and Baron, 1991). For instance, if only one pulse is detected from a particle, a phantom particle can be created when a pulse from another particle occur while the processor is open. The counting efficiency and the magnitude of coincidence effects of the APS is dependent on the gain of the photomultiplier tube, the thresholds of the two signal processors and the particle concentration. The photomultiplier tube gain and the 20 mV and 3 V thresholds are adjusted so that the counting efficiency is as high as possible for the LPP, without creating phantom particles, and the SPP creating so few phantom particles as possible. To maintain the size of the effects due to counting coincidence, the particle concentration is held at the same level for all experiments. During the experiments the particle concentration is constant, within $\pm 10\%$.

RESULTS AND DISCUSSION

The size calibration between the aerodynamic particle diameter measured with the APS and the projected area diameter measured with the optical microscope has been performed by Gudmundsson et al. (Gudmundsson et al., 1991). The calibration data is shown in table 1.

Impactor calculated aero- dynamic cutoff (μm)	Optical microscope		APS		
	number of measurements	projected area diameter (μm)	number of measurements	Without density effect correction aerodynamic particle diameter (μm)	With density effect correction aerodynamic particle diameter (μm)
1.95	4	2.10 (0.26)	6	1.76 (0.03)	1.64
4.05	3	4.17 (0.08)	5	3.96 (0.08)	3.47
10.08	5	9.02 (0.88)	4	9.59 (0.14)	7.90
20.08	4	15.68 (2.14)	5	17.54 (0.85)	14.05

Table 1. The 50% cutoff diameters of the impactors measured with the optical microscopy and the APS. The standard deviation of the 50% cutoff diameters is also given.

A pilot study of the deposition onto the eyes has been performed. The mannequin was facing the wind at a wind velocity of 1 m/s and the degree of turbulence was about 3%. The result is shown in figure 1. By visual examination it is obvious that most of the particles are deposited on the central area of the eye.

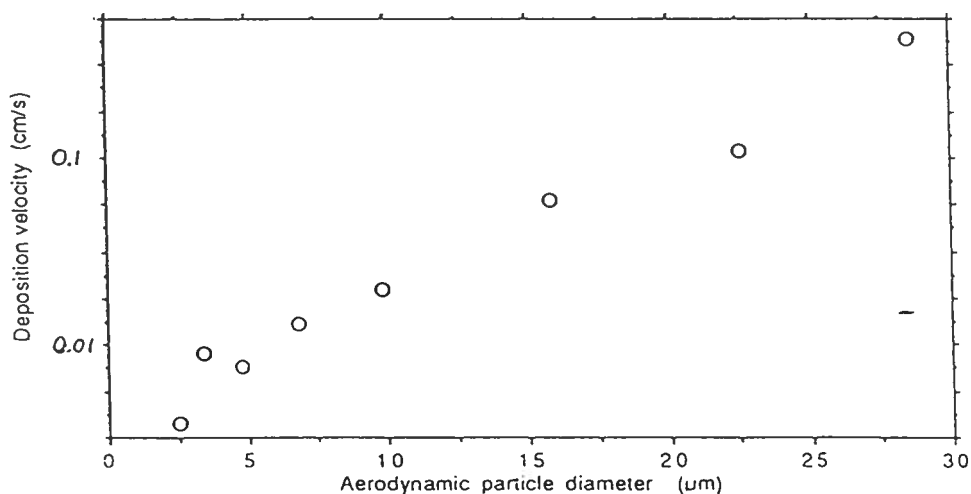


Figure 1. The deposition velocity onto a human eye as a function of the aerodynamic particle diameter. The mannequin is facing the wind. The air velocity is 1 m/s and the degree of turbulence is 3%.

To obtain quantitative results with high accuracy a careful calibration of the counting efficiency of the APS measurements has to be performed. The penetration losses in the sampling tube to the APS and the counting efficiency of the APS will be investigated.

REFERENCES

- Gudmundsson A., Petersen O.H., Schneider T. and Bohgard M. (1991). Contribution to European Aerosol Conference, September , Karlsruhe, Germany.
- Heitbrink W.A. and Baron P.A. (1991). Coincidence in time-of-flight aerosol spectrometers: phantom particle creation. Aerosol Sci. Technol., 14, 112-126.
- Remiarz R.J., Agarwal J.K., Quant F.R. and Sem G.J. (1983). Real-time aerodynamic particle size analyzer. In: Aerosols in the mining and industrial work environments (Marple V.A. and Liu B.Y.H., ed.), Vol 3, pp 879-895. Ann Arbor Science, Michigan.
-

NOVA and IV FINNISH AEROSOL SYMPOSIUM
at the Finnish Meteorological Institute (FMI)
Air Quality Department 14th and 15th of November 1991

EXPERIMENTAL DETERMINATION OF PARTICLE DEPOSITION
INTO THE HUMAN EYE

A. C. LINDHOLM¹, J. SCHNITZER², O. H. RUTENFRANZ²,
P. VINZENTI², M. RICHFIELD² AND K. K. KASSELHORN¹

¹Department of Working Environment, Lund Institute of Technology,
S-223 70, S-221 05 Lund, Sweden

²National Institute of Occupational Health, Tomtebodavägen 115,
S-210 01, Copenhagen, Denmark